


Dynamic and real-time display of running status

- Running status of reagent tray, sample tray and reaction tray
- Real-time monitoring of reagent residual volume
- Real-time diagnosis of system working status

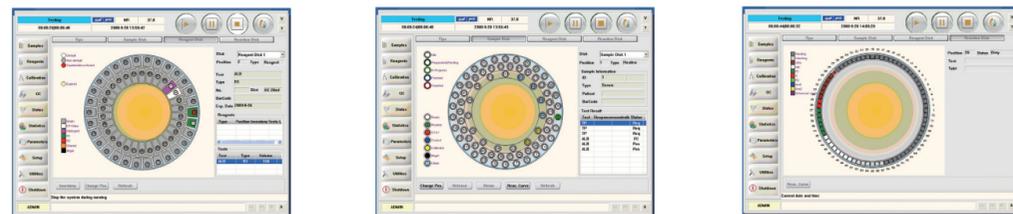


Flexible and convenient software function

- Template Modifying Software
Flexible to define various report templates for laboratory, and easy to import new template from Mindray or other users.
- Monitoring of various Samples
It is method to perform continuous glucose monitoring in subjects with impaired glucose tolerance or other multiple samples monitoring.
- Fast Emergency Detection
One-key STAT function makes it easy to perform an emergency test for operator.



Original reaction data record

- Real-time monitoring of reactions
- Simultaneously display reaction curves under primary and secondary wavelengths
- Detailed profile of alert messages



BS-380 Chemistry Analyzer

Technical Specifications

System Function:

Fully automated, Discrete, Random access for routine, STAT, Urine and homogeneous immuno assays;
STAT sample priority

Throughput: 300 tests / hour, up to 450 tests / hour with ISE

Measuring principles:

Absorbance photometry, Turbidimetry
End-point, Fixed-time, Kinetic, optional ISE
Single / Dual reagent chemistries, monochromatic / bichromatic
Linear / non-linear calibration

Programming:

User defined profiles and calculation

Sample Handling:

Sample tray: 75 positions for primary or secondary tubes and sample cups

Sample volume: 2~45µl, step by 0.1µl

Sample probe: Liquid level detection, vertical and horizontal collision protection

Probe cleaning: Interior and exterior automatic washing
Carry-over < 0.1%

Automatic sample dilution:

Pre-dilution and post-dilution ratio up to 1:150

Dilution vessel: Cuvette

Internal Bar Code Reader (optional):

Used for sample and reagent programming; applicable to various bar code systems including Codabar, ITF, Code128, Code 39, UPC / EAN, Code 93.
Bi-directional LIS interface

ISE Module (optional):

Optional selection of K⁺, Na⁺, Cl⁻

Throughput: Up to 225 tests per hour

Reagent Handling:

Reagent tray: 60 positions in refrigerated compartment (2~8°C)

Reagent volume: R1: 150~350µl, step by 1µl;

R2: 20~200µl, step by 1µl;

Reagent probe:

Liquid level detection, vertical and horizontal collision protection

Probe cleaning:

Interior and exterior automatic washing
Carry-over < 0.1%

Reaction System:

Reaction rotor: Rotating tray, 72 cuvettes with automatic washing

Cuvette: Optical length of 5mm

Reaction volume: 150~360µl

Operating temperature: 37°C

Temperature fluctuation: ±0.1°C

Mixing system: Integrated mixers system

Optical System:

Light Source: Halogen-tungsten lamp

Photometer: Reversed optics, grating photometry

Wavelength: 340nm, 380nm, 412nm, 450nm, 505nm, 546nm, 570nm, 605nm, 660nm, 700nm, 740nm, 800nm

Absorbance range: 0~3Abs

Resolution: 0.001Abs

Control and Calibration:

Calibration mode: Linear (one-point, two-point and multi-point), Logit-Log 4P, Logit-Log 5P, Spline, Exponential 5P, Polynomial 5P, Parabola
Control rules: Westgard multi-rule, Cumulative sum check, Twin plot

Operation Unit:

Operation system: Windows® XP Professional/Home SP2 or above
Windows® Vista Home/Business, Windows® 7
Interface: RS-232

Working Conditions:

Power Supply: AC 100~240V, 50 / 60Hz, 1000VA

Temperature: 15~30°C

Humidity: 35~85%

Water consumption: 10L/hour

Dimension: 990mm x 693mm x 1135mm (WxDxH)

Weigh: 200 Kg



BS-380 Chemistry Analyzer

Mindray Building, Keji 12th Road South, High-tech Industrial Park, Nanshan, Shenzhen 518057, P.R. China Tel: +86 755 8188 8998 Fax: +86 755 26582680 E-mail: intl-market@mindray.com www.mindray.com Mindray is listed on the NYSE under the symbol "MR"	mindray is a trademark of Shenzhen Mindray Bio-Medical Electronics Co., Ltd. ©2013 Shenzhen Mindray Bio-Medical Electronics Co., Ltd. All rights reserved. Specifications subject to changes without prior notice. P/N: ENG-B5380-21285x8-20130303	


BS-380 Chemistry Analyzer

- Discrete, random access, fully automated
- Constant 300 tests per hour, up to 450 tests per hour with ISE
- Onboard capacity of 75 sample positions, up to 58 chemistries plus 3 ions
- Refrigerated reagent compartment
- Automatic probe cleaning, liquid level detection, vertical and horizontal collision protection
- 8-step auto washing system
- 12 wavelengths: 340~800nm
- Automatic dilution for abnormal sample
- Internal bar code reader (optional)
- Bi-directional LIS interface



Multi-functional sample tray

- 75 sample positions
- Can be programmed into 5 virtual sample disks
- Primary tubes and various sample cups can be used
- Automatic dilution of high concentration sample
- Pre-dilution for samples
- Internal sample bar code reader (optional)



Reaction tray

- Test sequence optimization
- 150 μ L minimum total reaction volume
- Contains 72 reaction cuvettes
- Maintenance free heating system



High performance mixer design

- Integrated mixers system
- Optimized homogenization
- High precision mixer station to ensure excellent reaction conditions
- Standardized mixing procedures
- Separate mixer for individual reaction steps



Multi-functional sampling probes

- Interior and exterior probe washing
- Liquid level detection
- Collision protection
- Inventory monitoring
- Probe depth adjusted automatically



Washing station

- High-tech washing station to ensure accurate results and valid diagnostics
- Concentrated detergents to reduce carry-over
- 8-step auto washing station



Refrigerated reagent tray


- 58 reagent positions for R1, R2
- 24 hour non-stop cooling with Peltier element
- Ready-to-use liquid stable reagents
- Internal reagent bar code reader (optional)

BS-380 Chemistry Analyzer



Mindray solution for clinical chemistry

After more than 10 years of research and development on reagents, Mindray can now provide 48 parameters of dedicated reagents (more than 17 others are coming), covering hepatic, renal, cardiac, lipids, diabetes, pancreatitis, inorganic ions and immunoassays, etc., together with original calibrators with metrological traceability as well as controls for BS-380 chemistry analyzer.

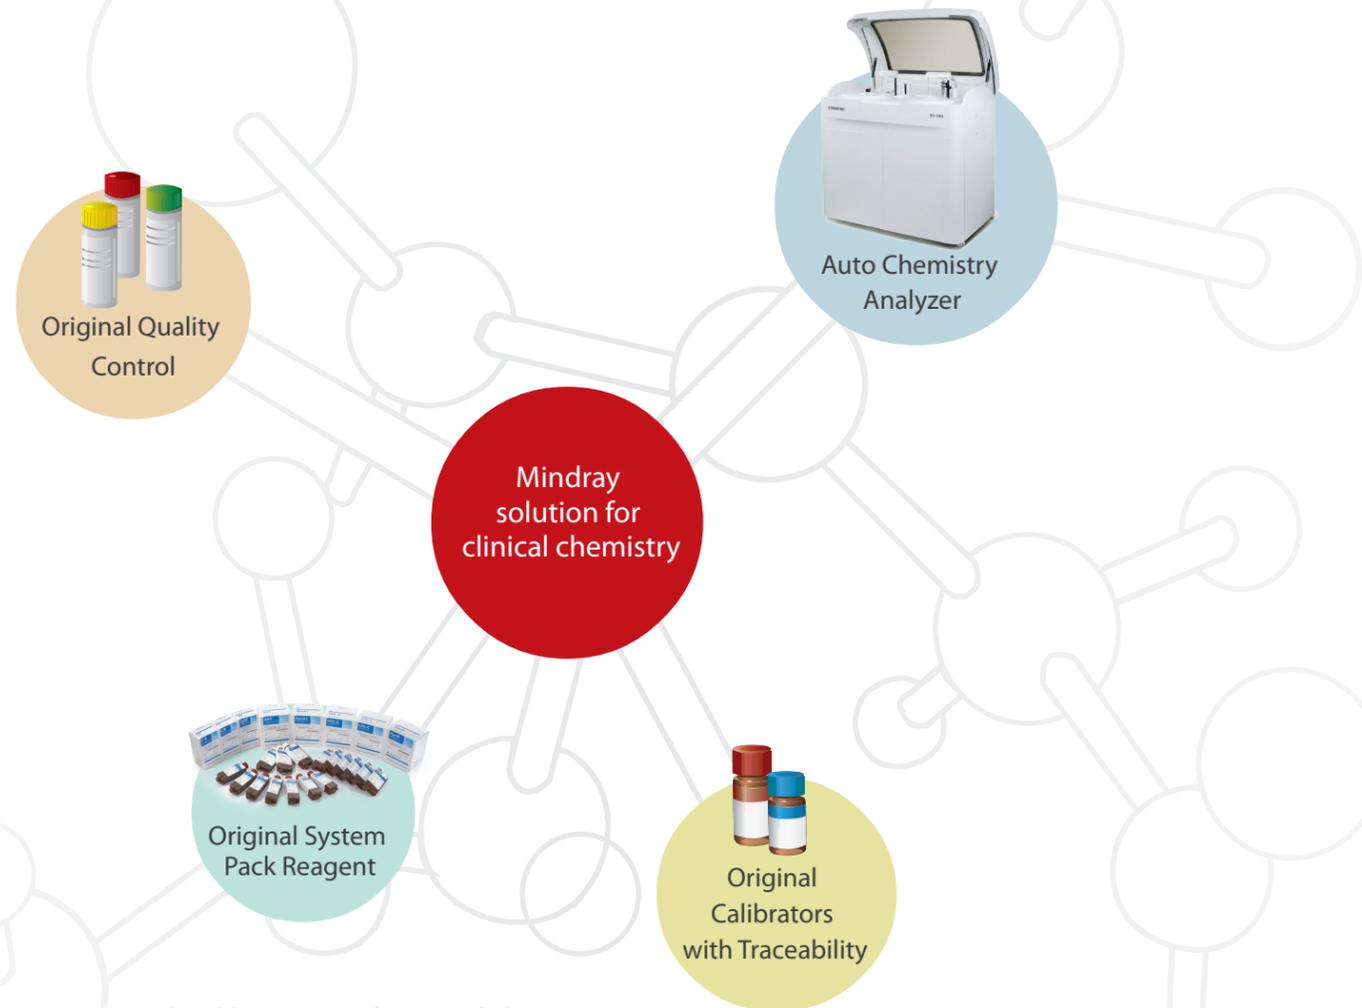

Original Calibrators with traceability:

Reference Method (Certified by 'Joint Committee for Traceability in Laboratory Medicine' (JCTLM))

- International Federation of Clinical Chemistry and Laboratory Medicine (IFCC)
- National Institute of Standards and Technology (NIST)
- Centers for Disease Control and Prevention (CDC, USA)
- American Association for Clinical Chemistry (AACC)

Reference Material

- Institute for Reference Materials and Measurements (IRMM) standards
- National Institute of Standards and Technology (NIST) standards
- World Health Organization (WHO) standards
- Japan Committee for Clinical Laboratory (JCCLS) standards

Chemistry Reagents

Hepatic

Alanine Aminotransferase (ALT)
 Aspartate Aminotransferase (AST)
 Alkaline Phosphatase (ALP)
 γ-Glutamyl Transferase (γ-GT)
 Direct Bilirubin (D-Bil) DSA Method
 Direct Bilirubin (D-Bil) VOX Method
 Total Bilirubin (T-Bil) DSA Method
 Total Bilirubin (T-Bil) VOX Method
 Total Protein (TP)
 Albumin (ALB)
 Total Bile Acids (TBA)
 Prealbumin (PA)
 Cholinesterase (CHE)
 Adenosine deaminase (ADA) *
 α-L-fucosidase (AFU) *
 5'-nucleotidase (5'-NT) *

Renal

Urea (UREA)
 Creatinine (CREA) Modified Jaffé Method
 Creatinine (CREA) Sarcosine Oxidase Method
 Uric Acid (UA)
 Carbon dioxide (CO₂)
 Microalbumin*
 β₂-Microglobulin (β₂-MG) *
 Cystatin C (CysC) *

Cardiac

Creatine Kinase (CK)
 Creatine Kinase-MB (CK-MB)
 Lactate Dehydrogenase (LDH)
 α-Hydroxybutyrate Dehydrogenase (α-HBDH)
 Homocysteine (HCY)
 Myoglobin*

Ferrum

Iron (Fe)
 Ferritin (FER) *
 Transferrin (TRF) *
 Total iron binding capacity / unsaturated iron binding capacity (TIBC/UIBC) *

Lipids

Total Cholesterol (TC)
 Triglycerides (TG)
 HDL-Cholesterol (HDL-C)
 LDL-Cholesterol (LDL-C)
 Apolipoprotein A1 (ApoA1)
 Apolipoprotein B (ApoB)
 Lipoprotein(a) [LP(a)]

Pancreatitis

α-Amylase (α-AMY)
 Lipase (LIP)

Diabetes

Glucose (Glu) GOD-POD Method
 Glucose (Glu) HK Meth
 Hemoglobin A1c (HbA1c)
 Fructosamine (FUN)

Inorganic ions

Calcium (Ca)
 Magnesium (Mg)
 Phosphate Inorganic (P)

Rheumatism

High sensitivity C-reactive protein (hs-CRP) *
 Rheumatoid Factor (RF)
 Antibodies Against Streptolysin O (ASO)

Immune

Immunoglobulin A (IgA)
 Immunoglobulin G (IgG)
 Immunoglobulin M (IgM)
 Immunoglobulin E (IgE) *
 Complement C3 (C3)
 Complement C4 (C4)
 C-Reactive Protein (CRP)

Others

Glucose-6-phosphate dehydrogenase (G6PD) *
 D-dimer*
 Angiotensin converting enzyme (ACE) *
 Retinol binding protein (RBP) *
 D3-hydroxybutyric acid (D3-HB) *

* Coming soon